



HPLC columns


# Connected chromatography solutions

Low-flow columns and accessories

# Introduction

Low-flow chromatography is ideal when detailed sample information is required from small sample volumes, such as proteomic, metabolomic, and intact protein analysis. The Thermo Scientific range of nano-, capillary-, and micro-flow columns offer excellent sensitivity and resolution in easy-to-use formats.


- Thermo Scientific™  $\mu$ PAC™ Neo HPLC Columns
- Thermo Scientific™ EASY-Spray™ HPLC Columns
- Thermo Scientific™ Double nanoViper™ HPLC Columns

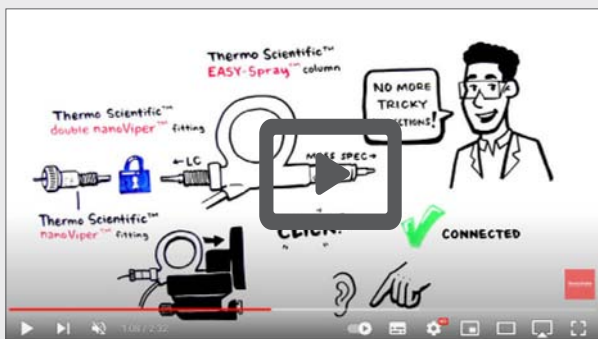




**Video:** Low-flow HPLC columns connectivity


# Contents

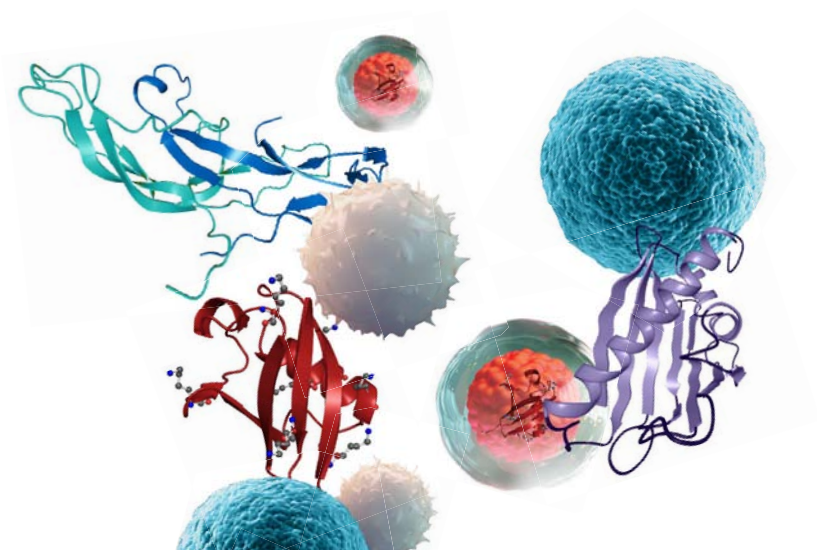μPAC Neo HPLC columns	5
<hr/>	
EASY-Spray HPLC columns	8
Bottom-up proteomics	9
Top-down proteomics	10
<hr/>	
Double nanoViper HPLC columns	12
Bottom-up proteomics	13
Top-down proteomics	14
<hr/>	



# Column selection guide

	Pillar array column format	Packed bed column format	
	Thermo Scientific™ $\mu$ PAC™ Neo HPLC Columns	Thermo Scientific™ EASY-Spray™ HPLC Columns	Thermo Scientific™ Double nanoViper™ HPLC Columns
Technology			
Benefits	<p><b>Ultimate separation</b></p> <ul style="list-style-type: none"> <li>• Excellent retention time stability</li> <li>• A unique combination of performance and reliability to get the highest sample coverage every time</li> <li>• Separate emitters</li> <li>• Compatible with all low-flow U/HPLC instruments</li> </ul>	<p><b>Ease-of-use</b></p> <ul style="list-style-type: none"> <li>• Click-and-spray connect with Thermo Scientific™ EASY-Spray™ Source</li> <li>• Thermo Scientific™ nanoViper™ connections</li> <li>• Integrated column and emitter</li> <li>• Integrated temperature control</li> <li>• For use with Thermo Scientific™ mass spectrometry systems</li> </ul>	<p><b>Analytical flexibility</b></p> <ul style="list-style-type: none"> <li>• Universal Thermo Scientific™ nanoViper™ Fingertight Fittings for column inlet and outlet</li> <li>• Simple zero-dead-volume (ZDV) connections</li> <li>• Separate emitters</li> <li>• Compatible with all low-flow U/HPLC instruments</li> </ul>
Application areas/chemistries	<p>Deliver excellent column-to-column reproducibility with flow rate flexibility. Ideally suited for proteomic analyses of HPLC separations up to 450 bar.</p> <ul style="list-style-type: none"> <li>• 50 cm column: 15–60 min gradient time</li> <li>• 110 cm column: 90–150 min gradient time</li> <li>• 50 cm Low Load single cell analysis: 15–60 min gradient time</li> <li>• High Throughput: &lt;15 min gradient time, for up to 180 samples/day</li> </ul>	<p><b>Bottom-up proteomic applications</b> The Thermo Scientific™ PepMap™ Neo UHPLC Columns are a recent addition to our portfolio. PepMap Neo columns are packed to higher pressure, which provides 1500 bar pressure rating, improved column-to-column consistency, and increased efficiency.</p> <p><b>Top- and middle-down proteomic applications</b> The Thermo Scientific™ MAbPac™ Capillary Reversed-Phase HPLC Column is best suited for the characterization of intact proteins in top- and middle-down proteomic applications where sample amount is limited.</p>	

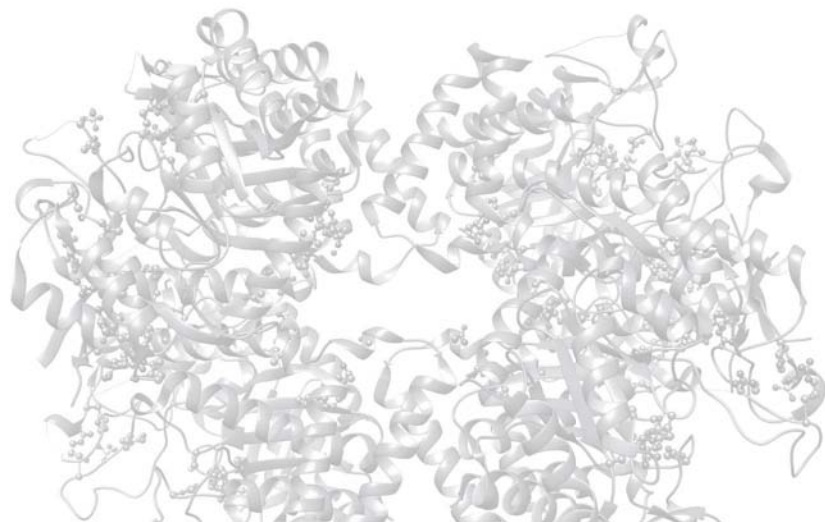

# μPAC Neo HPLC columns



The μPAC Neo columns are specifically suited for bottom-up proteomic applications where separation performance is critical to the success of the analysis. Our μPAC Neo HPLC columns offer highest resolution and peak capacities for complex biological samples. The unique μ-pillar backbone improves column-to-column reproducibility and robustness, providing more confidence in analytical results.

## Additional reading

Links	Type	Description
	<b>Reference guide</b>	Chromatography consumables reference guide for low-flow LC-MS proteomic research
	<b>Flyer</b>	Enabling high sensitivity LC-MS analysis for bottom-up and top-down proteomic research
	Learn more <a href="https://thermofisher.com/lowflowHPLCcolumns">thermofisher.com/lowflowHPLCcolumns</a>	

## Choose a μPAC Neo HPLC column when:

- Highest resolution and peak capacities is required
- Your samples span a wide concentration range
- Highest LC-MS sensitivity is needed
- You want to speed up your runtimes
- LC-MS robustness is needed
- You want an increased column lifetime
- You prefer working at much lower back pressures than with packed bed columns
- It is important to compare results from experiments spanning over time or geographical location

## What makes μPAC Neo HPLC columns special?


### The unique separation path provides:

- μ-pillar stationary backbone, micromachined in a silicon wafer
- Flow path designed for highest analyte concentration during elution
- Extra high-resolution separations, using up to 110 cm column lengths
- Low back pressure separations, improving column and emitter robustness
- Perfect match with single cell proteomics sample amounts




# μPAC Neo HPLC columns Continued

## Velocity Label-free Quantitation (LFQ) Data Independent Acquisition (DIA) Platform

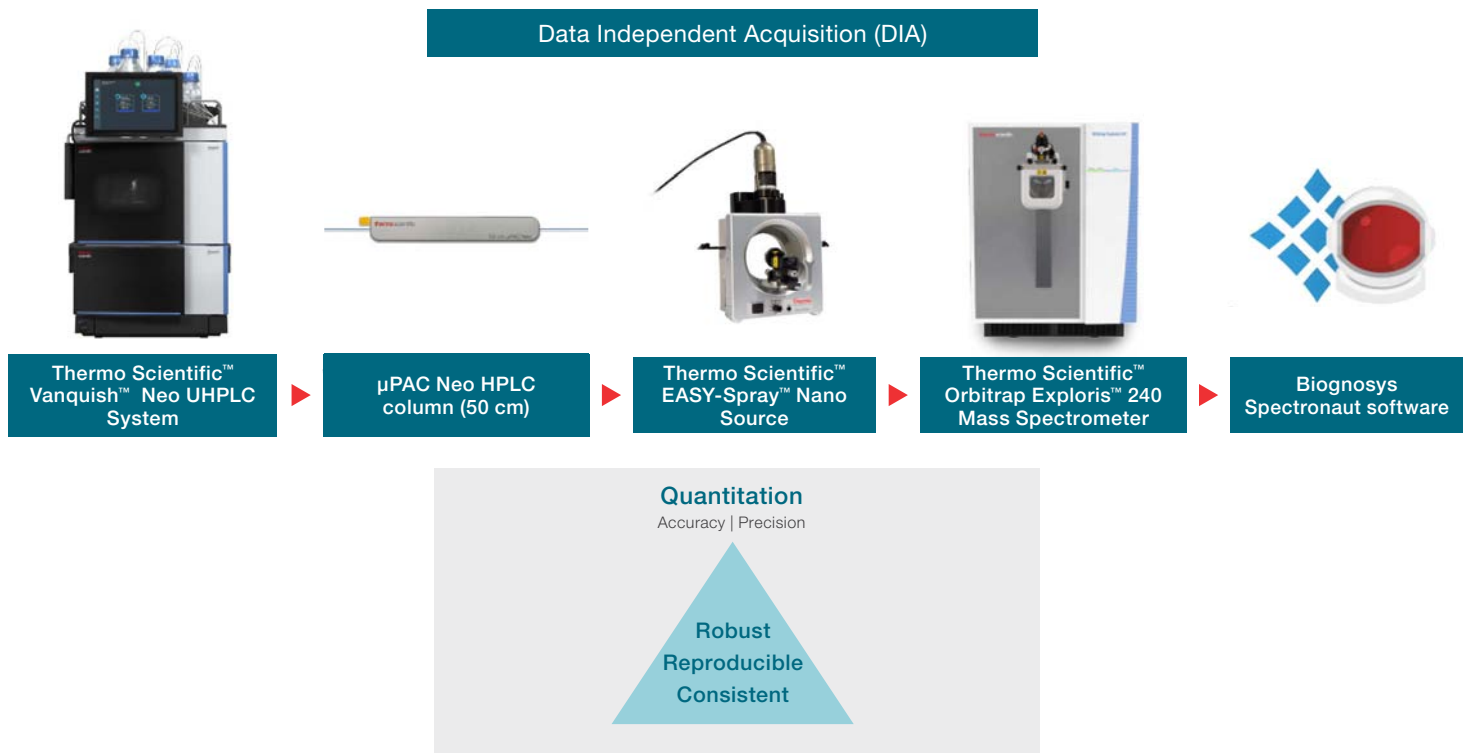

**Figure 1. Graphical schematic of HR-DIA workflow for label-free quantitation of two- and three-proteome mixtures.** The different components of the workflow are depicted on the top. The main goal of the setup is the quantitative performance at high sample throughput while delivering robust and reproducible results to make it a perfect fit for large scale clinical and biomarker discovery studies.

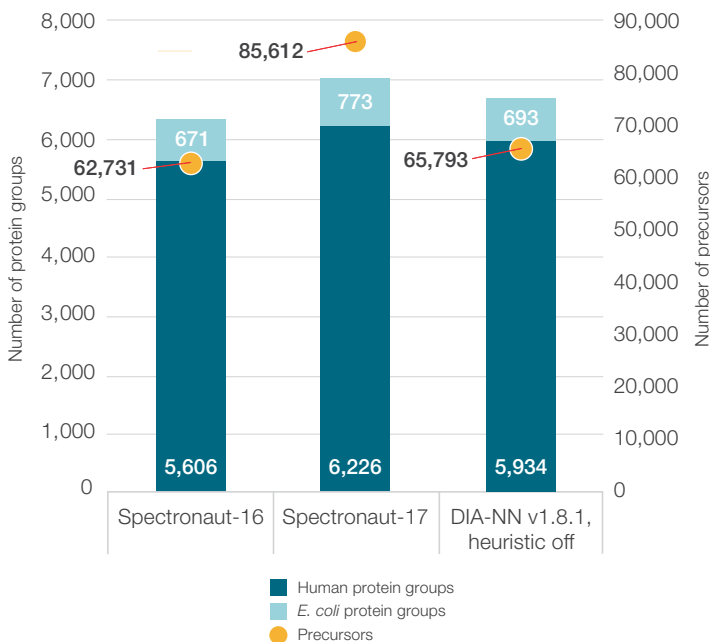

**Figure 2. HR-DIA Workflow delivers confident proteome coverage utilizing next generation library-free analysis approaches.** Bar graph comparison of protein group (human and *E. coli*) and precursor (total) numbers identified in 12 runs of two-proteome mix by use of three different software packages. Data analysis has been done by library-free analysis. All protein group results are filtered for 1% experiment-wide FDR.

# μPAC Neo HPLC columns Continued



## Ordering information


Description	Pillar dimensions (μm)	Interpillar distance (μm)	Column length (cm)	Flowrate range (nL/min)	Cat. no
Thermo Scientific 50 cm μPAC Neo Column	2.5	1.25	50	100-750	<a href="#">COL-NANO050NEOB</a>
Thermo Scientific 110 cm μPAC Neo Column	2.5	1.25	110	100-750	<a href="#">COL-NANO110NEOB</a>
Thermo Scientific 50 cm μPAC Neo Low Load column	2.5	1.25	50	100-750	<a href="#">COL-LOLO050NEOB</a>
Thermo Scientific μPAC Neo High Throughput Column	3.0	2	5.5	250-2500	<a href="#">COL-CAPHTNEOB</a>

## Ordering information

Description	Pillar dimensions (μm)	Interpillar distance (μm)	Column length (cm)	Cat. no
Thermo Scientific™ μPAC™ Neo Trapping Column	5	2.5	1	<a href="#">COL-TRPLOLONEOB2</a>

## Ordering information

Description	Pillar dimensions (μm)	Details	For use with	Cat. no
Thermo Scientific™ EASY-Spray™ Nano Emitters	10	Bullet type without transfer line	EASY-Spray ion-source	<a href="#">ES993</a>

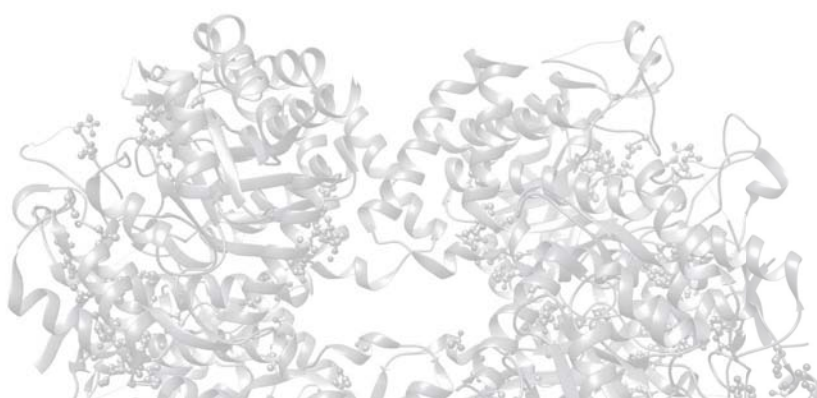

# EASY-Spray HPLC columns



Ensure robust nano- and capillary-flow LC-MS analysis using Thermo Scientific EASY-Spray HPLC Columns. The integrated column/emitter design eliminates dead volume and is temperature-controlled for maximum reliability and performance. Rigorously tested to ensure maximum quality, these columns deliver maximum simplicity and ease-of-use. The capillary-flow HPLC columns provide sensitive protein, peptide, and monoclonal antibody (MAb) separation. They give proteomic researchers more than ever before: more throughput, more sensitivity, more separation power, and more ease of use.

## Additional reading

Links	Type	Description
	Reference guide	Chromatography consumables reference guide for low-flow LC-MS proteomic research
	Flyer	Enabling high sensitivity LC-MS analysis for bottom-up and top-down proteomic research
	Learn more <a href="https://thermofisher.com/lowflowHPLCcolumns">thermofisher.com/lowflowHPLCcolumns</a>	

## Choose an EASY-Spray column when:

- You want simple connections with an EASY-Spray source. This is ideal for novice and experienced users
- Sample amount is limited
- Analytical UHPLC does not provide sufficient sensitivity
- Workflow simplicity is key
- High sensitivity is required to identify proteins and peptides at low expression levels
- Analyses are done in a targeted and untargeted way for screening and verification

## What makes an EASY-Spray column special?

Unique design provides uncompromised performance in an ease-of-use format for nano and capillary LC-MS analysis

### Features for optimum data quality:

- Simple connection to the LC and Thermo Scientific MS instruments
- Precision machined and positioned glass emitters
- Integrated nanoViper zero-dead-volume (ZDV) unions
- Integrated temperature control



### Video:

Thermo Scientific EASY-Spray  
150 mm LC columns







### PepMap Neo HPLC columns

The Thermo Scientific™ EASY-Spray™ PepMap™ Neo UHPLC Columns are perfect for bottom-up proteomic applications. Packed at higher pressure and rated to 1500 bar, they provide consistent column-to-column performance, long column lifetime, and excellent efficiency. These benefits are true at any pressure.

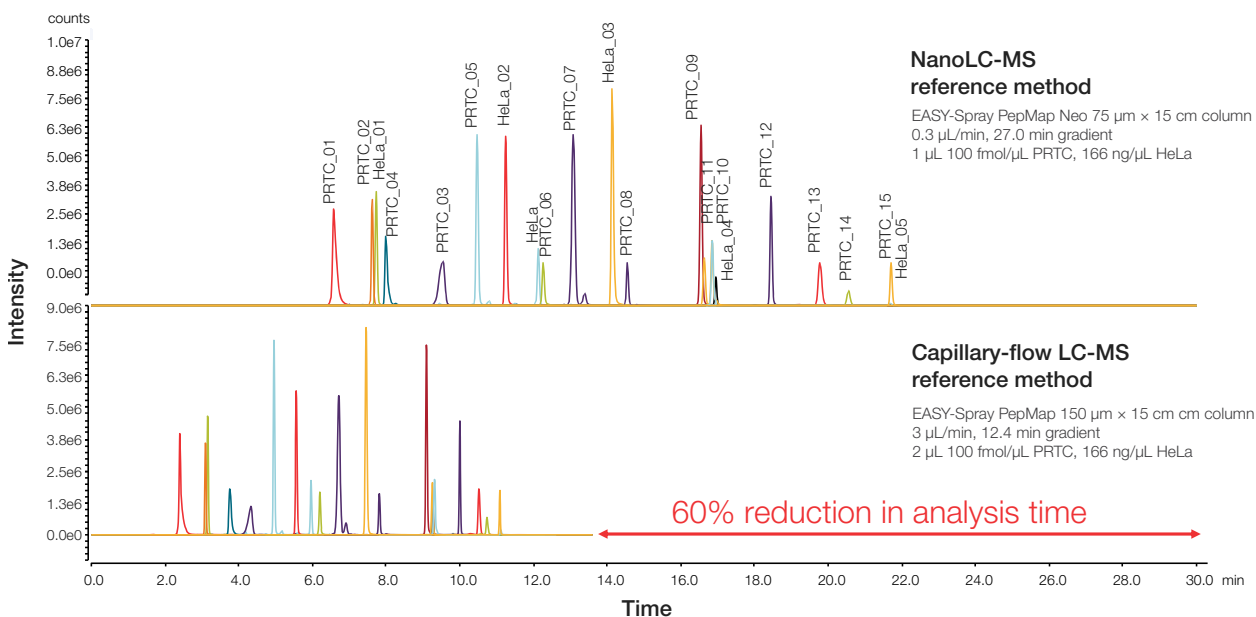


Figure 3. The 60% reduction in total analysis time allows increasing the sample throughput moving from the nano- to the capillary-flow LC-MS method



#### Ordering information for bottom-up proteomic applications

Description	Length (mm)	Column ID ( $\mu\text{m}$ )	Cat. no
EASY-Spray PepMap Neo UHPLC Columns	150	75	<a href="#">ES75150PN</a>
	500	75	<a href="#">ES75500PN</a>
	750	75	<a href="#">ES75750PN</a>





## Top-down proteomics

### MABPac Capillary Reversed Phase HPLC Column

The Thermo Scientific™ MABPac™ Capillary Reversed Phase capillary column is best suited for the characterization of intact proteins in top-down proteomic, clinical, and anti-doping applications where sample amount is limited or sensitivity is crucial.

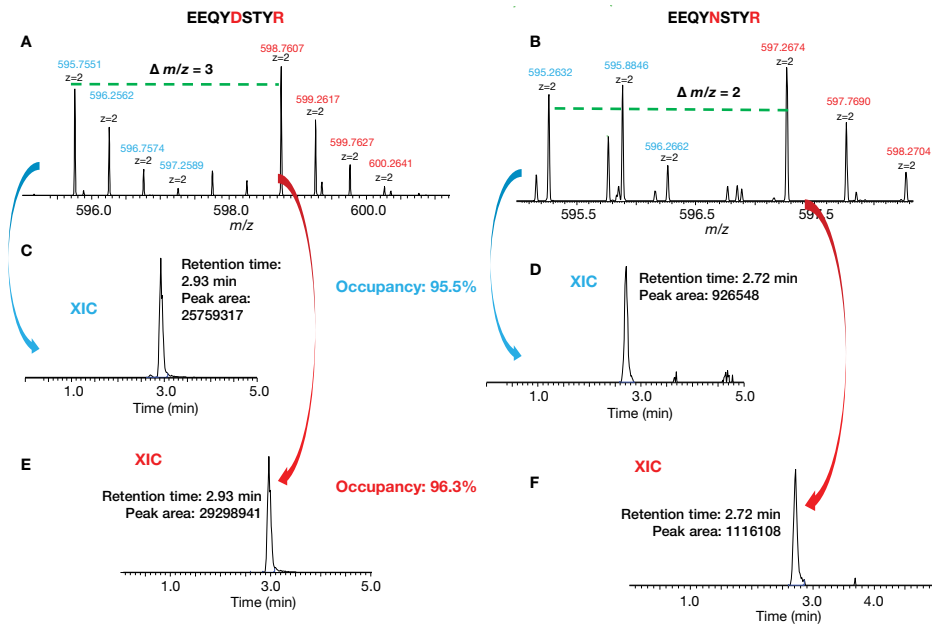


Figure 4. Calculation of site occupancy of N306 in Fab glycosylated mAb



Ordering information for top-down proteomic applications

Description	Length (mm)	Column ID (μm)	Cat. no
EASY-Spray HPLC Column	150	150	<a href="#">ES907</a>



# EASY-Spray HPLC columns Continued



## EASY-Spray accessories

For the best performance from your EASY-Spray column consider investing in these accessories.




### Ordering information

Description	Union type	Particle size (μm)	Column ID (μm)	Media bed length (mm)	Trap length (mm)	Cat. no
Thermo Scientific™ PepMap™ Neo Trap Cartridge	N/A	5	300	5	N/A	<a href="#">174500</a>
	Nut/sleeve	5	200	20	150	<a href="#">164213</a>
	Nut/sleeve	5	100	20	150	<a href="#">164199</a>
Thermo Scientific™ Acclaim™ PepMap™ 100 C18 HPLC Column, Trap Column	Double nanoViper	5	100	20	150	<a href="#">164750</a>
	Double nanoViper	3	75	20	150	<a href="#">164535</a>
	Double nanoViper	3	75	20	70	<a href="#">164946</a>

### Ordering information

Description	For use with	Cat. no
Thermo Scientific™ PepMap™ Neo Trap Cartridge Holder, PEEK Tubing, and nanoViper™ Fittings	Low-flow PepMap columns	<a href="#">174502</a>

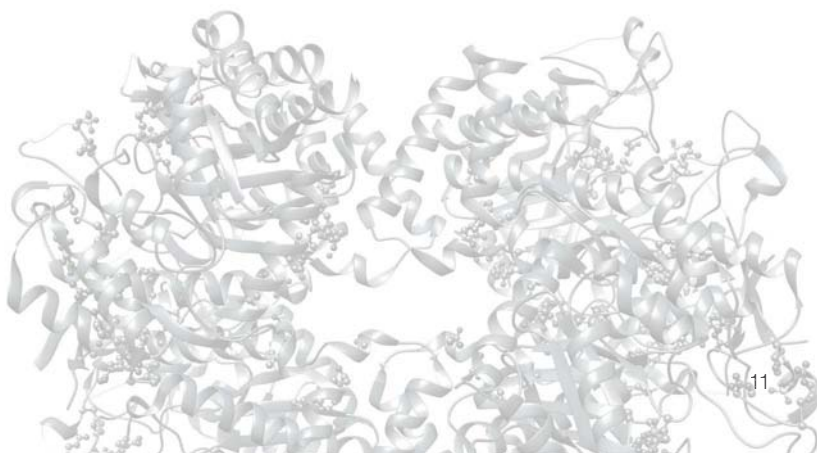

# Double nanoViper columns



The Thermo Scientific™ Viper™ and Thermo Scientific™ nanoViper™ Fingertight Fitting Systems provide tool-free connections designed to be used for the entire fluidic pathway in LC systems to improve chromatographic results.

Virtually without any dead-volume, Viper and nanoViper fittings combine usability with high performance. Viper and nanoViper connections can be used on all standard LC modules, valves, and columns quickly, independent of different connection geometries and system backpressures. Dedicated capillary kits for standard LC system configurations and application-specific setups enable high qualitative and reproducible results for all flow rates and pressure ranges.

## Additional reading

Links	Type	Description
	<b>Reference guide</b>	Chromatography consumables reference guide for low-flow LC-MS proteomic research
	<b>Flyer</b>	Enabling high sensitivity LC-MS analysis for bottom-up and top-down proteomic research
	<b>Product specifications</b>	Viper and nanoViper Fingertight Fitting Systems
	Learn more <a href="https://www.thermofisher.com/lowflowHPLCcolumns">thermofisher.com/lowflowHPLCcolumns</a>	

## Choose these columns when:


- Maximum flexibility is required
- Changing the emitter and column independently is important



## What makes these columns special?


**These stand-alone nano-, capillary-, and micro-flow columns are:**

- Designed with single nanoViper and double nanoViper fingertight fittings for trouble-free connection
- For robust separation in proteomics research, drug discovery, and high-throughput proteomics laboratories

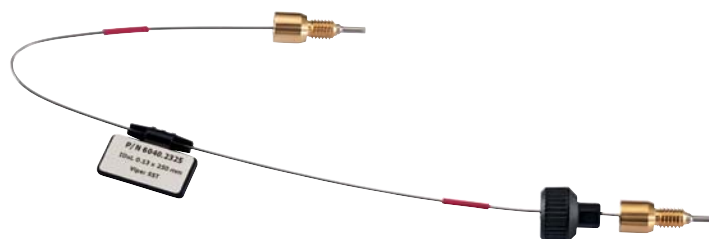

## Video:

Discover a better LC connection



### Double nanoViper PepMap Neo UHPLC columns

Separate challenging peptide mapping samples with Thermo Scientific™ Double nanoViper™ PepMap™ Neo UHPLC Columns. These columns feature easy connectivity, high reproducibility, and excellent separations. Our Neo columns are packed to higher pressure and provide 1500 bar pressure capability, improved column-to-column consistency, and increased efficiency. The column media is manufactured and selected to exacting standards and packed at high pressure, resulting in enhanced peak symmetry, resolution, and column-to-column reproducibility that allows you to obtain greater sample coverage and sample insights.

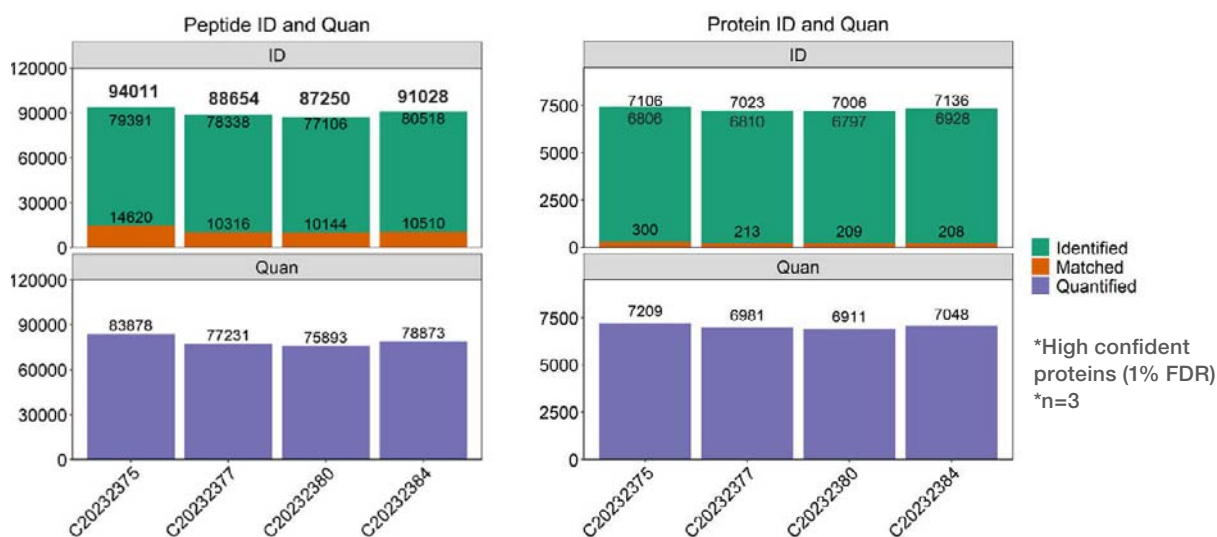


Figure 5. Reproducible identification and quantification of HeLa peptides and proteins over 4 EASY-Spray PepMap Neo columns while using the Vanquish Neo UHPLC system coupled with the Orbitrap Exploris 480 mass spectrometer



#### Ordering information for bottom-up proteomic applications

Format	Length (mm)	Column ID (µm)	Cat. no
Double nanoViper PepMap Neo UHPLC Columns	150	75	<a href="#">DENV75150PN</a>
	500	75	<a href="#">DENV75500PN</a>
	750	75	<a href="#">DENV75750PN</a>



# Double nanoViper columns Continued

## Top-down proteomics



### MABPac Capillary Reversed Phase HPLC Column

The Thermo Scientific MABPac Capillary Reversed Phase column is best suited for the characterization of intact proteins in top-down proteomic, clinical, and anti-doping applications where sample amount is limited or sensitivity is crucial.

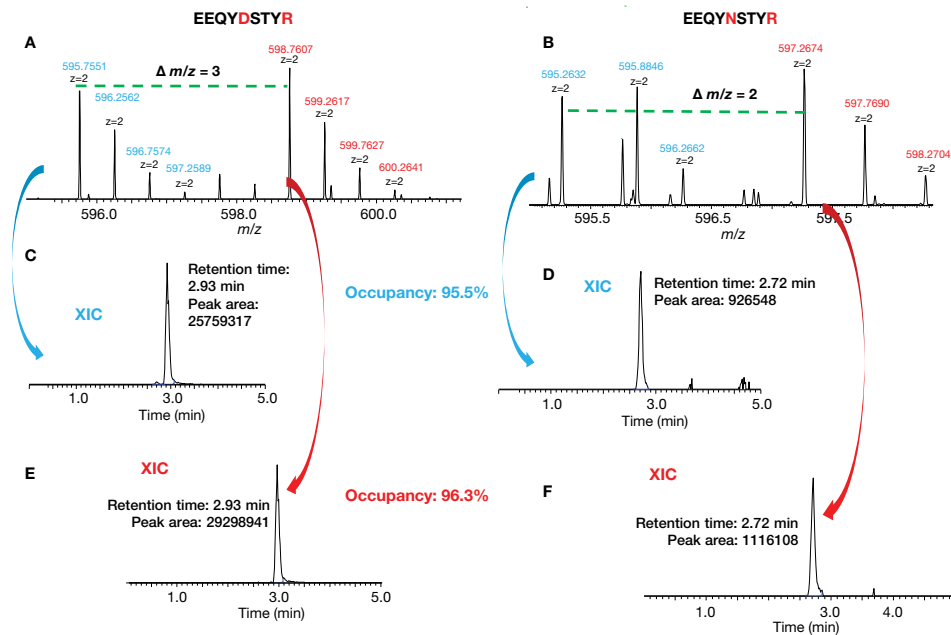


Figure 6. Calculation of site occupancy of N306 in Fab glycosylated mAb



#### Ordering information for top-down proteomic applications

Format	Length (mm)	Column ID ( $\mu\text{m}$ )	Cat. no.
MABPac Capillary Reversed Phase HPLC Column	150	150	<a href="#">164947</a>



# Double nanoViper columns Continued



## LC-MS connection accessories and emitters

These emitters, nanoViper tubing kits, and unions offer easy connection from your LC system to an EASY-Spray source.



### Ordering information

Description	For use with	Part number
Viper and nanoViper Fingertight Fittings Accessories		<a href="#">6040.2304</a>
nanoViper Fingertight Fittings, 20 µm x 550 mm	Double nanoViper columns	<a href="#">6041.5260</a>
EASY-Spray Nano Emitter, 10 µm		<a href="#">ES993</a>
EASY-Spray Capillary Emitter, 15 µm		<a href="#">ES994</a>

## Traps and accessories

For the best performance from your double nanoViper column consider investing in these nanotraps.



### Ordering information

Description	Union type	Particle size (µm)	Column ID (µm)	Media bed length (mm)	Trap length (mm)	Cat. no
Thermo Scientific™ PepMap™ Neo Trap Cartridge	N/A	5	300	5	N/A	<a href="#">174500</a>
	Nut/sleeve	5	200	20	150	<a href="#">164213</a>
	Nut/sleeve	5	100	20	150	<a href="#">164199</a>
Thermo Scientific™ Acclaim™ PepMap™ 100 C18 HPLC Column, Trap Column	Double nanoViper	5	100	20	150	<a href="#">164750</a>
	Double nanoViper	3	75	20	150	<a href="#">164535</a>
	Double nanoViper	3	75	20	70	<a href="#">164946</a>



Expect reproducible results with sample prep, columns and vials



Don't see what you need? We would be happy to discuss your specific requirements. Please contact your local sales representative for custom orders.

 Learn more at [thermofisher.com/lowflowHPLCcolumns](https://thermofisher.com/lowflowHPLCcolumns)